

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 122 505

Pellet-burettes, 50 ml, lat. needle valve, AS, conf. cert.




Batch: 07-20

Serial:

Measuring Nr. 43677

Batch size: 23

Volume:	50,0000 ml	30,0000 ml	10,0000 ml
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	50,0031 ml	30,0154 ml	10,0100 ml
Deviation:	0,0106 ml	0,0134 ml	0,0089 ml
Precision (CV):	0,0212 %	0,0448 %	0,0887 %

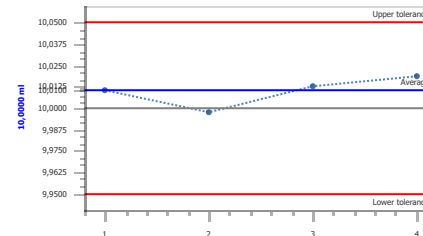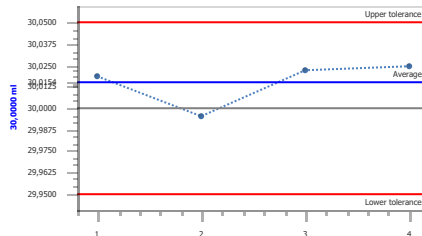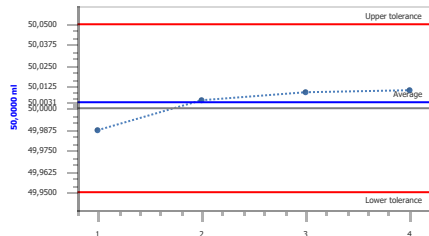

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	22.01.2021
Balance:	Sartorius - LE244S-OCE

DE-M