

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 122 505

Pellet-burettes, 50 ml, lat. needle valve, AS, conf. cert.




Batch: 20-23

Serial:

Measuring Nr. 66905

Batch size: 20

Volume:	50,000 ml	30,000 ml	10,000 ml
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	50,0168 ml	30,0198 ml	10,0216 ml
Deviation:	0,0067 ml	0,0033 ml	0,0065 ml
Precision (CV):	0,0134 %	0,0111 %	0,0647 %

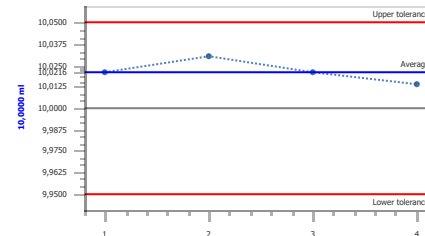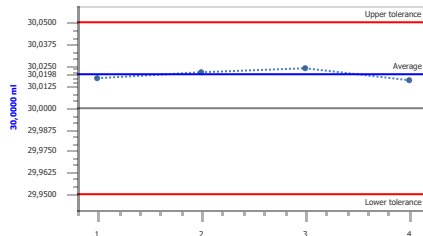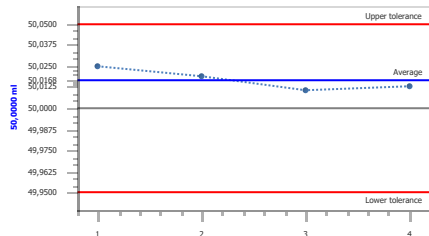

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	23.04.2024
Balance:	Sartorius - LE244S-OCE

DE-M