

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 122 508

Pellet-burettes, 50 ml, lat. needle valve, AS, conf. cert.




Batch: 01-18

Serial:

Measuring Nr.: 22231

Batch size: 30

Volume:	50,000 ml	30,000 ml	10,000 ml
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	50,0330 ml	30,0444 ml	10,0348 ml
Deviation:	0,0070 ml	0,0022 ml	0,0039 ml
Precision (CV):	0,0139 %	0,0075 %	0,0387 %

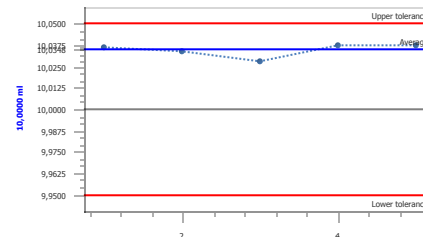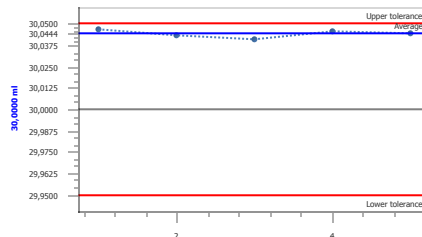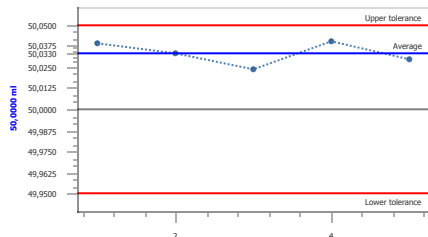

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator: 4

Date: 12.07.2018

Balance: Sartorius - LE244S-OCE

DE-M