

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 122 508

Pellet-burettes, 50 ml, lat. needle valve, AS, conf. cert.




Batch: 45-21

Serial:

Measuring Nr. 52146

Batch size: 20

Volume:	50,0000 ml	30,0000 ml	10,0000 ml
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	49,9933 ml	29,9993 ml	10,0221 ml
Deviation:	0,0075 ml	0,0144 ml	0,0048 ml
Precision (CV):	0,0150 %	0,0481 %	0,0476 %

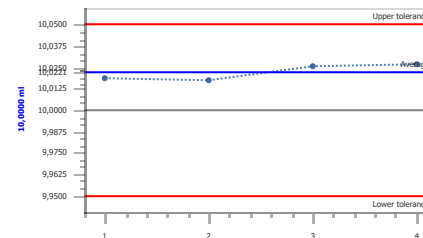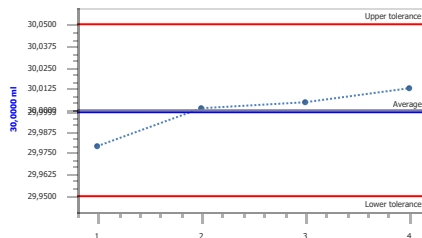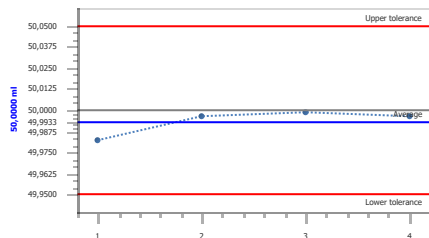

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	15.02.2022
Balance:	Sartorius - LE244S-OCE

DE-M