

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 124 105

Pellet-burettes, 10 ml, amber glass, AS, conf. cert.




Batch: 23-21

Serial:

Measuring Nr. 74473

Batch size: 15

Volume:	10,0000 ml	6,0000 ml	2,0000 ml
Tolerance:	± 0,0200 ml	± 0,0200 ml	± 0,0200 ml
Average value:	9,9996 ml	6,0011 ml	2,0040 ml
Deviation:	0,0053 ml	0,0050 ml	0,0008 ml
Precision (CV):	0,0533 %	0,0836 %	0,0420 %

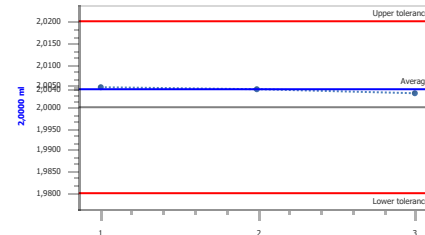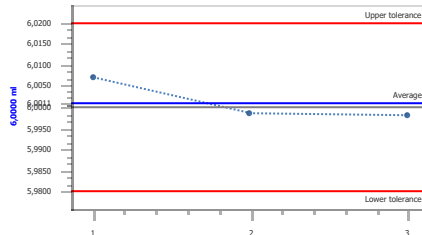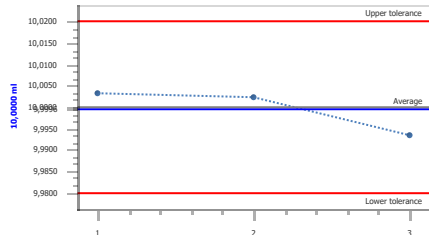

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

03.09.2025

Balance:

Sartorius -
LE244S-OCE

DE-M