Certificate of performance


witeg GERMANY

ISO 9001 CERTIFIED

Article:	**3 124 505**
Pellet-burettes, 50 ml, amber glass, AS, conf. cert.	

Batch:	19-26	**Serial:**	
Measuring Nr.	80449	**Batch size:**	10

Volume:	**50,0000 ml**	**30,0000 ml**	**10,0000 ml**
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	49,9867 ml	29,9782 ml	10,0107 ml
Deviation:	0,0108 ml	0,0108 ml	0,0145 ml
Precision (CV):	0,0217 %	0,0359 %	0,1454 %

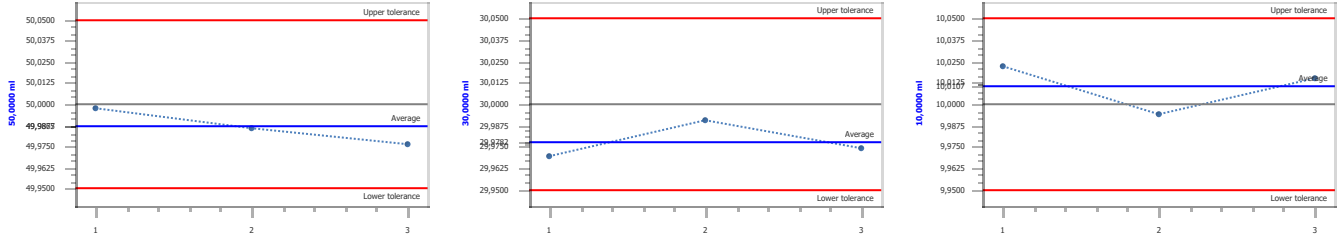

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH
Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	29.10.2026
Balance:	Sartorius - LE244S-0CE

DE-M