

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 152 255

Univ. automatic burettes, 25 ml, AS, conf. cert.




Batch: 24-18

Serial:

Measuring Nr.: 25681

Batch size: 6

Volume:	25,0000 ml	15,0000 ml	5,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	24,9962 ml	14,9956 ml	5,0040 ml
Deviation:	0,0088 ml	0,0053 ml	0,0085 ml
Precision (CV):	0,0351 %	0,0350 %	0,1695 %

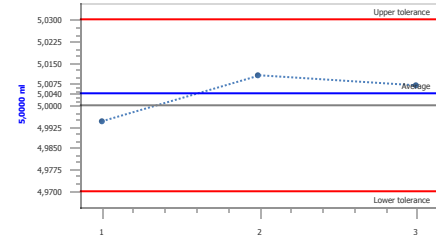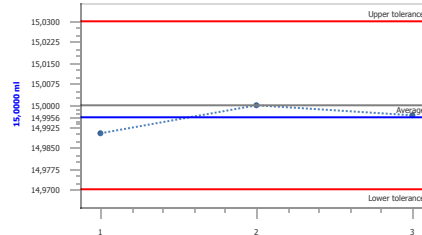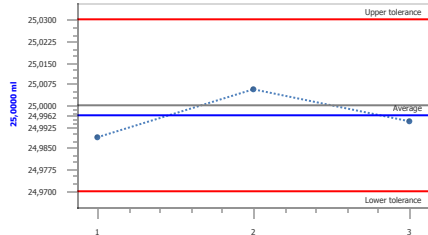

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	20.11.2018
Balance:	Sartorius - LE244S-OCE

