

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 154 254

Universal autom. burettes, 25 ml, AS, conf. cert.




Batch: 44-21

Serial:

Measuring Nr.: 56233

Batch size: 20

Volume:	25,0000 ml	15,0000 ml	5,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	24,9904 ml	14,9892 ml	5,0155 ml
Deviation:	0,0071 ml	0,0058 ml	0,0003 ml
Precision (CV):	0,0284 %	0,0384 %	0,0058 %

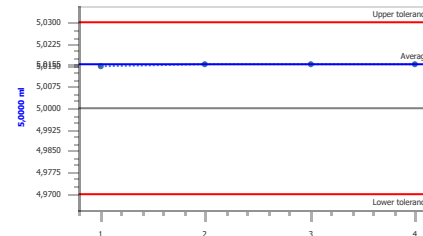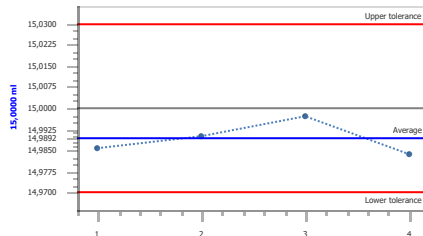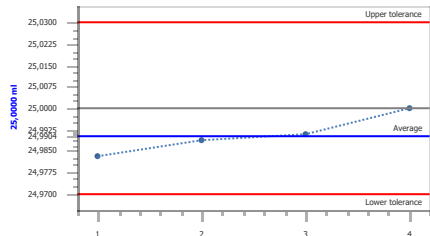

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	25.05.2022
Balance:	Sartorius - LE244S-OCE

