

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 154 255

Universal autom. burettes, 25 ml, AS, conf. cert.




Batch: 44-21

Serial:

Measuring Nr.: 74021

Batch size: 3

Volume:	25,0000 ml	15,0000 ml	5,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	24,9988 ml	14,9988 ml	5,0099 ml
Deviation:	0,0023 ml	0,0039 ml	0,0021 ml
Precision (CV):	0,0093 %	0,0258 %	0,0426 %

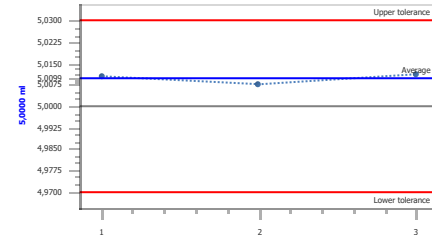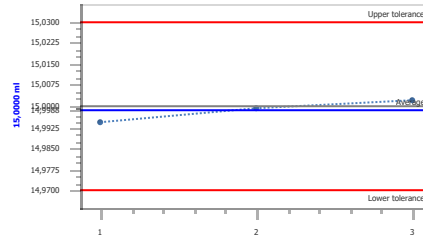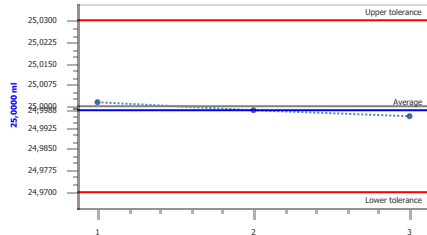

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	05.08.2025
Balance:	Sartorius - LE244S-OCE

