

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 372 023

Micro burette, 2 ml, str. stopc., PTFE, AS, conf. cert.




Batch: 13-23

Serial:

Measuring Nr. 71185

Batch size: 10

Volume:	2,0000 ml	1,2000 ml	0,4000 ml
Tolerance:	± 0,0100 ml	± 0,0100 ml	± 0,0100 ml
Average value:	2,0033 ml	1,2025 ml	0,3964 ml
Deviation:	0,0008 ml	0,0021 ml	0,0028 ml
Precision (CV):	0,0418 %	0,1741 %	0,6984 %

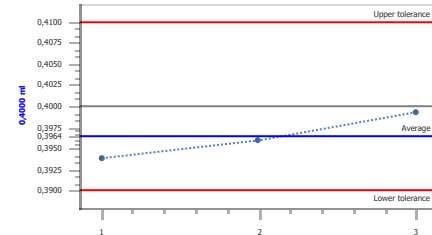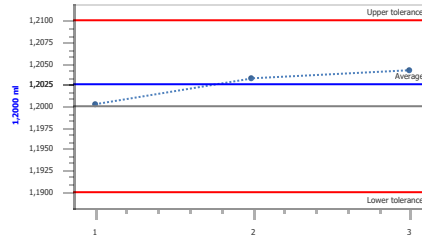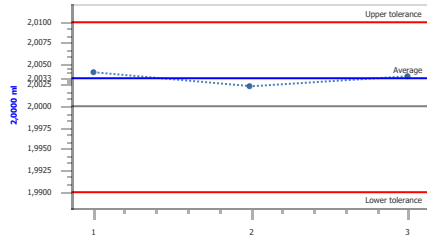

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	77
Date:	10.12.2024
Balance:	Sartorius - LE244S-OCE

