

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 372 052

Micro burettes, 5 ml, straight stopc., AS, conf. cert.




Batch: 46-24

Serial:

Measuring Nr. 71415

Batch size: 6

Volume:	5,0000 ml	3,0000 ml	1,0000 ml
Tolerance:	± 0,0100 ml	± 0,0100 ml	± 0,0100 ml
Average value:	5,0025 ml	3,0046 ml	1,0012 ml
Deviation:	0,0022 ml	0,0026 ml	0,0020 ml
Precision (CV):	0,0436 %	0,0880 %	0,1954 %

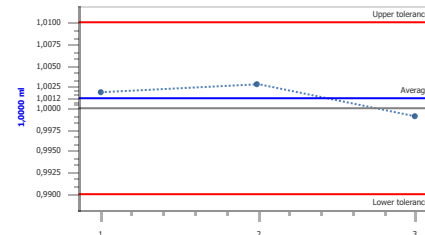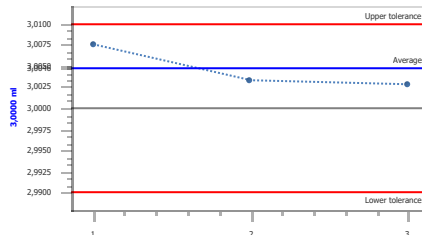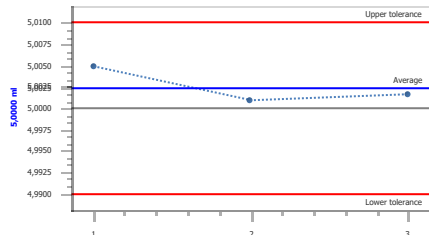

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	22.01.2025
Balance:	Sartorius - LE244S-OCE

