

Certificate of performance



ISO 9001
CERTIFIED

Article: 4711632

Burettes, 50 ml, lateral valve, Schellb., AS, conf. cert.




Batch: 31-22

Serial:

Measuring Nr. 60445

Batch size: 50

Volume:	50,0000 ml	30,0000 ml	10,0000 ml
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	50,0126 ml	29,9968 ml	9,9984 ml
Deviation:	0,0170 ml	0,0061 ml	0,0106 ml
Precision (CV):	0,0341 %	0,0203 %	0,1063 %

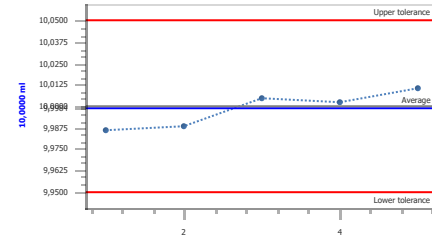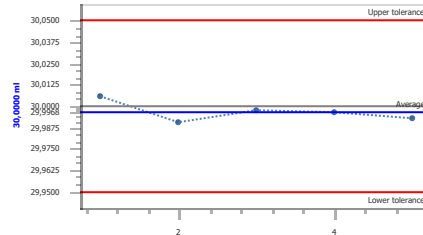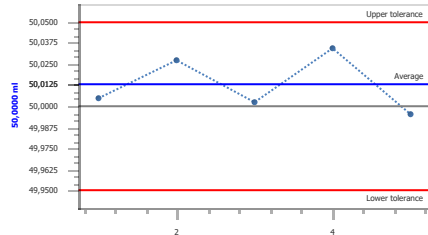

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	24.11.2022
Balance:	Sartorius - MSE224S-0CE -DU

