

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 000

Graduated cylinder, 5:0,1 ml, A, conf. cert.




Batch: 50-19

Serial:

Measuring Nr.: 35295

Batch size: 262

Volume:	1,0000 ml	3,0000 ml	5,0000 ml
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	0,9959 ml	3,0067 ml	5,0040 ml
Deviation:	0,0103 ml	0,0111 ml	0,0139 ml
Precision (CV):	1,0295 %	0,3712 %	0,2781 %

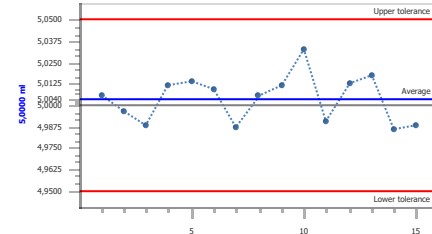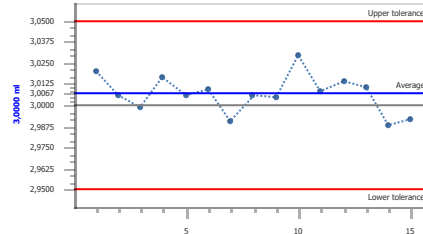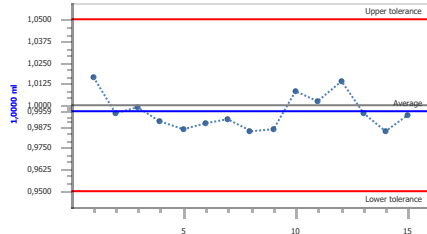

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	18.12.2019
Balance:	Sartorius - LE244S-OCE

