

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 715 001 USP

**Grad. cylinder, 10:0,2 ml, USP, A, conf. cert.**




**Batch:** 27-21

**Serial:**

**Measuring Nr.** 47787

**Batch size:** 280

Volume:	2,0000 ml	6,0000 ml	10,0000 ml
<b>Tolerance:</b>	± 0,1000 ml	± 0,1000 ml	± 0,1000 ml
<b>Average value:</b>	1,9910 ml	5,9997 ml	10,0039 ml
<b>Deviation:</b>	0,0200 ml	0,0137 ml	0,0122 ml
<b>Precision (CV):</b>	1,0003 %	0,2283 %	0,1215 %

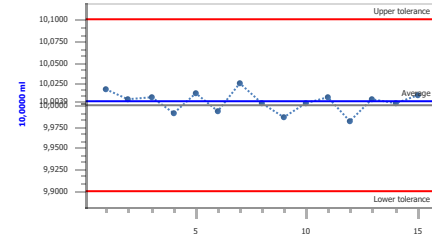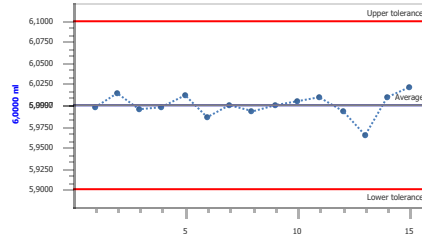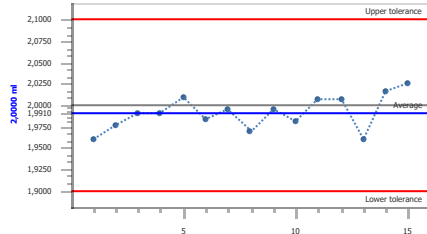

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	7
<b>Date:</b>	08.07.2022
<b>Balance:</b>	Sartorius - LE244S-OCE

