

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 001 USP

Grad. cylinder, 10:0,2 ml, USP, A, conf. cert.




Batch: 11-23

Serial:

Measuring Nr. 62034

Batch size: 280

Volume:	2,0000 ml	6,0000 ml	10,0000 ml
Tolerance:	± 0,1000 ml	± 0,1000 ml	± 0,1000 ml
Average value:	1,9928 ml	5,9885 ml	9,9836 ml
Deviation:	0,0204 ml	0,0171 ml	0,0168 ml
Precision (CV):	1,0219 %	0,2854 %	0,1684 %

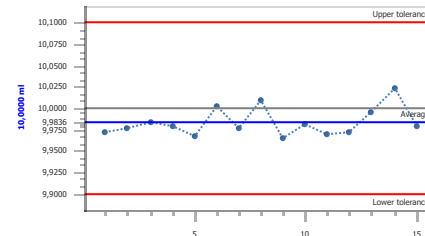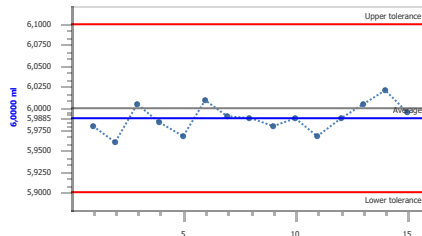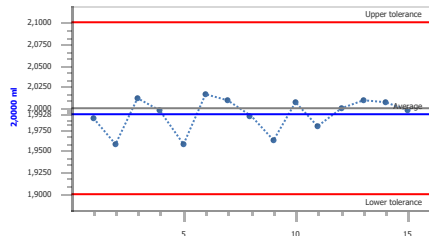

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	21.03.2023
Balance:	Sartorius - LE244S-OCE

DE-M