

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 005 USP

Grad.cylinder, 50:1 ml, USP, A, conf.cert.




Batch: 05-21

Serial:

Measuring Nr. 44350

Batch size: 150

Volume:	10,000 ml	30,000 ml	50,000 ml
Tolerance:	± 0,2500 ml	± 0,2500 ml	± 0,2500 ml
Average value:	10,0106 ml	30,0244 ml	50,0076 ml
Deviation:	0,0217 ml	0,0417 ml	0,0645 ml
Precision (CV):	0,2165 %	0,1389 %	0,1291 %

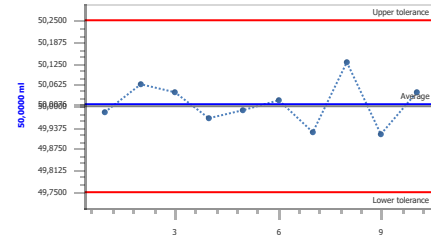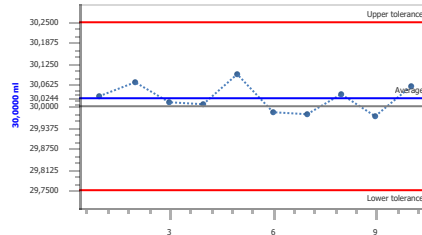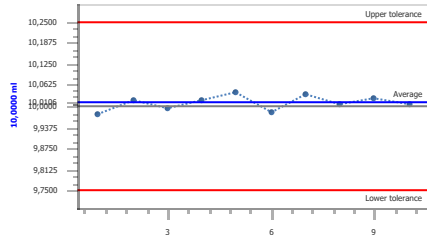

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	10.02.2021
Balance:	Sartorius - LE244S-OCE

