
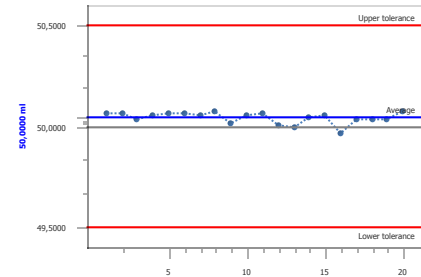
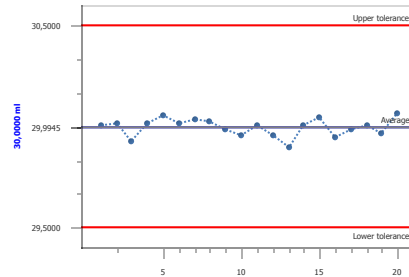


Certificate of performance

Article number 3 715 005
 Batch 50-16
 Serial number
 Measuringnr./Batch size 10017 / 500
 Balance Precisa - XT 220A
 Operator 4
 Date 20.12.2016

Graduated cylinder class A

Volume	10,0000ml	30,0000ml	50,0000ml
Tolerance	0,5000ml	0,5000ml	0,5000ml
Measuring volume	9,9519 ml	29,9945 ml	50,0427 ml
Deviation	-0,4807 %	-0,0183 %	0,0854 %
Number of measurings	20	20	20

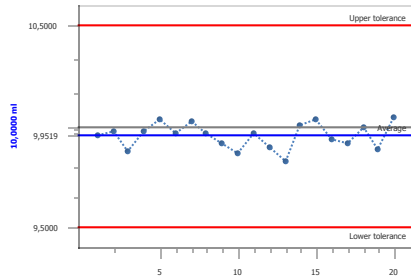

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
 97877 Wertheim
 Germany
 +49 (0) 9342 / 9301-0
 | info@witeg.de

