

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 005

Graduated cylinders, 50:1 ml, A, conf. cert.




Batch: 48-25

Serial:

Measuring Nr. 75996

Batch size: 280

Volume:	10,000 ml	30,000 ml	50,000 ml
Tolerance:	± 0,5000 ml	± 0,5000 ml	± 0,5000 ml
Average value:	10,1614 ml	30,1204 ml	50,0787 ml
Deviation:	0,0703 ml	0,0615 ml	0,0484 ml
Precision (CV):	0,7029 %	0,2051 %	0,0969 %

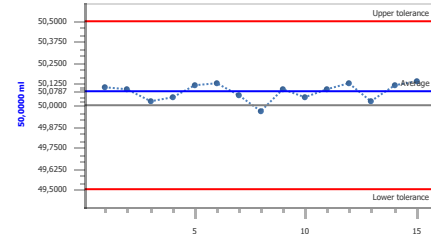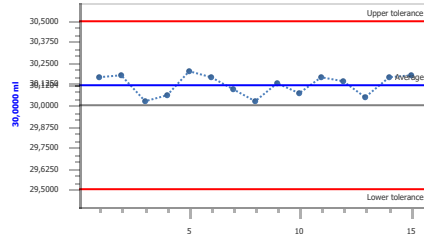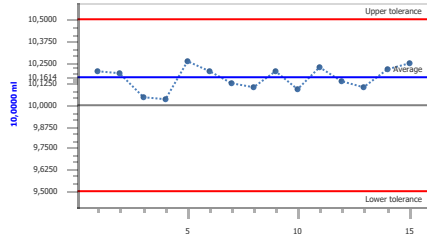

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	11.12.2025
Balance:	Sartorius - MSE224S-0CE -DU

