

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 005

Graduated cylinders, 50:1 ml, A, conf. cert.




Batch: 13-26

Serial:

Measuring Nr. 77289

Batch size: 1200

Volume:	10,000 ml	30,000 ml	50,000 ml
Tolerance:	± 0,5000 ml	± 0,5000 ml	± 0,5000 ml
Average value:	10,0251 ml	30,0508 ml	50,0224 ml
Deviation:	0,0756 ml	0,0589 ml	0,0426 ml
Precision (CV):	0,7563 %	0,1963 %	0,0852 %

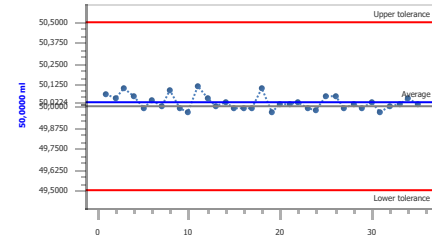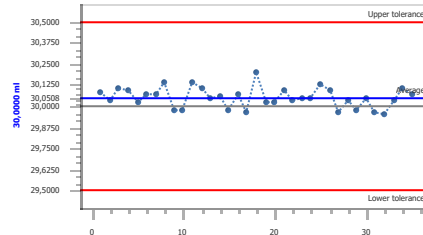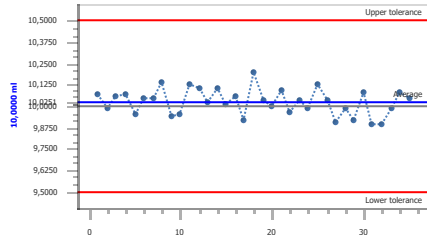

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	02.04.2026
Balance:	Sartorius - MSE224S-0CE -DU

