

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 010 BL

Grad. cylinder, 100:1,0 ml, blue grad., A, conf. cert.




Batch: 18-26

Serial:

Measuring Nr. 78135

Batch size: 500

Volume:	20,0000 ml	60,0000 ml	100,0000 ml
Tolerance:	$\pm 0,5000$ ml	$\pm 0,5000$ ml	$\pm 0,5000$ ml
Average value:	20,0292 ml	60,0197 ml	100,0416 ml
Deviation:	0,1088 ml	0,0890 ml	0,0545 ml
Precision (CV):	0,5441 %	0,1484 %	0,0545 %

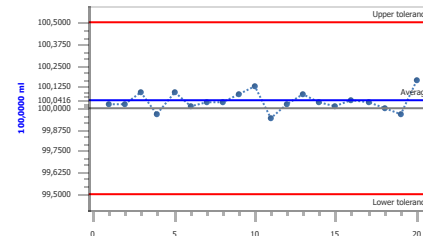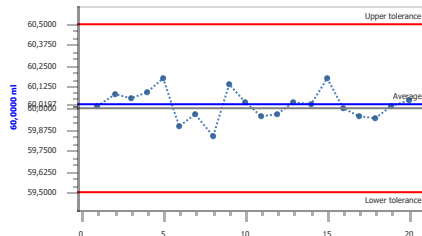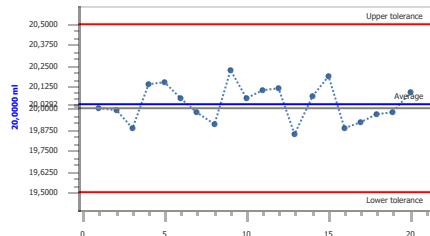

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

28.05.2026

Balance:

Sartorius -
LE244S-OCE

DE-M