

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 715 010 USP

**Graduated cylinders, 100:1 ml, USP, A, conf. cert.**




**Batch:** 42-21

**Serial:**

**Measuring Nr.** 49945

**Batch size:** 500

Volume:	20,000 ml	60,000 ml	100,000 ml
<b>Tolerance:</b>	± 0,5000 ml	± 0,5000 ml	± 0,5000 ml
<b>Average value:</b>	20,0754 ml	60,0285 ml	100,0178 ml
<b>Deviation:</b>	0,0728 ml	0,0777 ml	0,0614 ml
<b>Precision (CV):</b>	0,3639 %	0,1295 %	0,0614 %

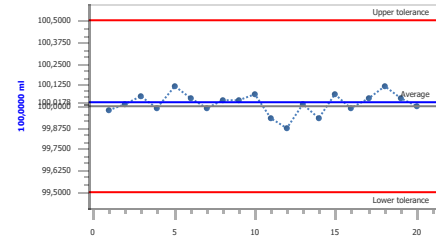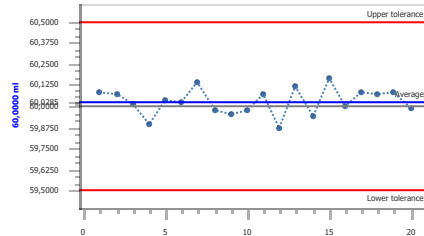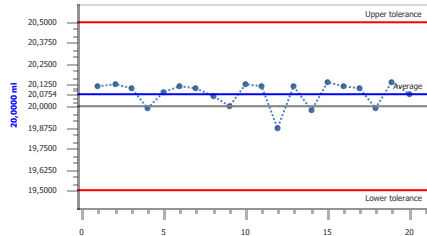

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	7
<b>Date:</b>	25.10.2021
<b>Balance:</b>	Sartorius - LE244S-OCE

