

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 010

Graduated cylinder, 100:1,0 ml, A, conf. cert.




Batch: 29-20

Serial:

Measuring Nr. 39156

Batch size: 2399

Volume:	20,000 ml	60,000 ml	100,000 ml
Tolerance:	± 0,5000 ml	± 0,5000 ml	± 0,5000 ml
Average value:	19,9036 ml	59,9587 ml	100,0050 ml
Deviation:	0,1091 ml	0,0993 ml	0,0973 ml
Precision (CV):	0,5457 %	0,1654 %	0,0973 %

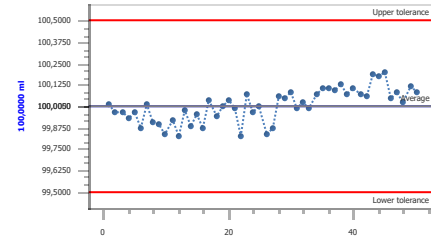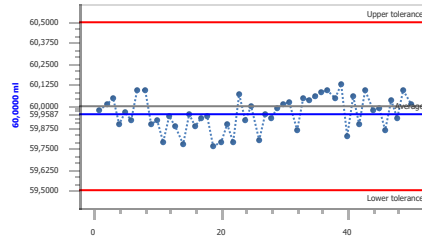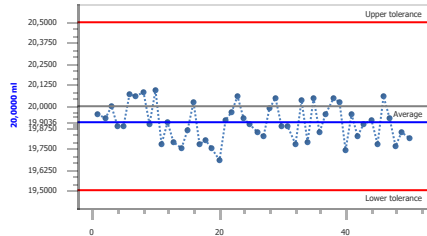

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	22.07.2020
Balance:	Sartorius - LE244S-OCE

