

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 025 BL USP

Grad. cylinder, 250:2 ml, blue, USP, A, conf. cert.




Batch: 42-20

Serial:

Measuring Nr. 41709

Batch size: 100

Volume:	50,0000 ml	150,0000 ml	250,0000 ml
Tolerance:	± 1,0000 ml	± 1,0000 ml	± 1,0000 ml
Average value:	49,9769 ml	150,0239 ml	249,9460 ml
Deviation:	0,1740 ml	0,1702 ml	0,1120 ml
Precision (CV):	0,3479 %	0,1135 %	0,0448 %

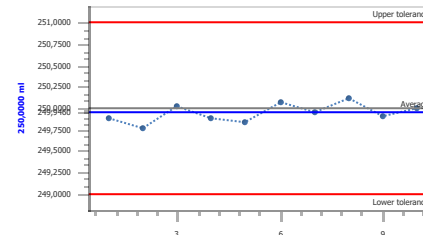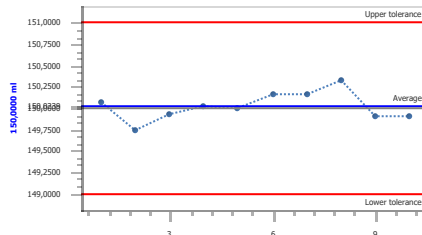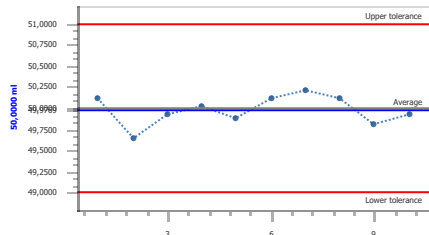

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	27.10.2020
Balance:	Sartorius - LA 1200 S

