

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 025 BL

Grad. cylinder, 250 ml, blue grad., A, conf. cert.




Batch: 46-17

Serial:

Measuring Nr. 15741

Batch size: 500

Volume:	50,0000 ml	150,0000 ml	250,0000 ml
Tolerance:	± 1,0000 ml	± 1,0000 ml	± 1,0000 ml
Average value:	49,8758 ml	150,0066 ml	250,0837 ml
Deviation:	0,2196 ml	0,1318 ml	0,1151 ml
Precision (CV):	0,4392 %	0,0879 %	0,0460 %

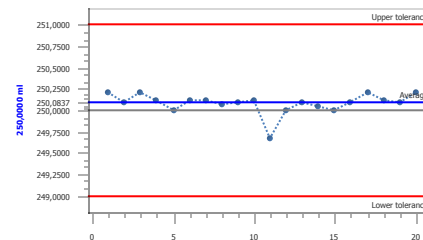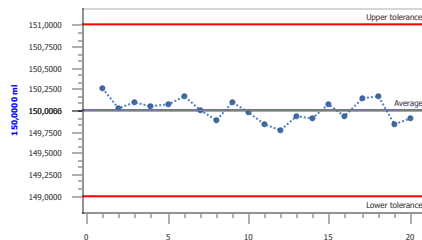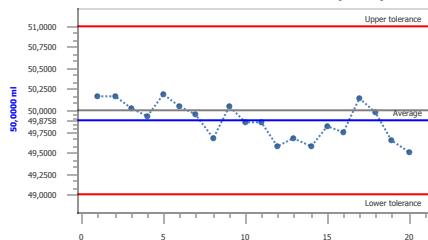

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	16.11.2017
Balance:	Sartorius - LA 1200 S

