

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 025 BL

Grad. cylinder, 250:2 ml, blue grad., A, conf. cert.




Batch: 43-19

Serial:

Measuring Nr. 33892

Batch size: 280

Volume:	50,0000 ml	150,0000 ml	250,0000 ml
Tolerance:	± 1,0000 ml	± 1,0000 ml	± 1,0000 ml
Average value:	50,0693 ml	150,1575 ml	250,1955 ml
Deviation:	0,3311 ml	0,2112 ml	0,1248 ml
Precision (CV):	0,6622 %	0,1408 %	0,0499 %

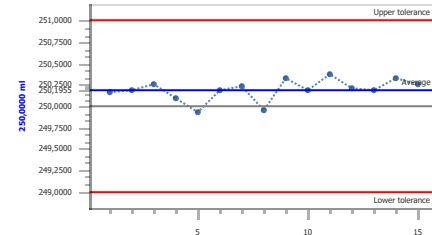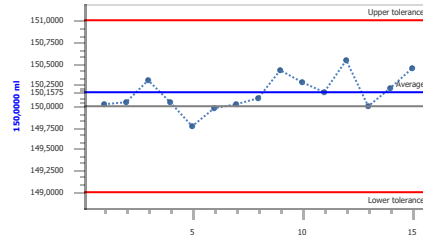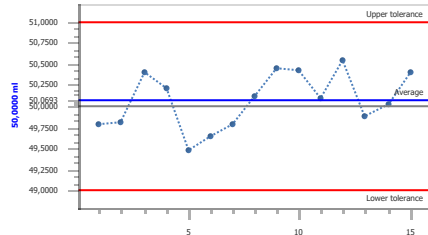

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	28.10.2019
Balance:	Sartorius - LA 1200 S

