

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 715 025 BL

**Grad. cylinder, 250:2 ml, blue grad., A, conf. cert.**




**Batch:** 43-23

**Serial:**

**Measuring Nr.** 65081

**Batch size:** 499

Volume:	50,0000 ml	150,0000 ml	250,0000 ml
<b>Tolerance:</b>	± 1,0000 ml	± 1,0000 ml	± 1,0000 ml
<b>Average value:</b>	49,7457 ml	149,9320 ml	250,2463 ml
<b>Deviation:</b>	0,2190 ml	0,2610 ml	0,2072 ml
<b>Precision (CV):</b>	0,4381 %	0,1740 %	0,0829 %

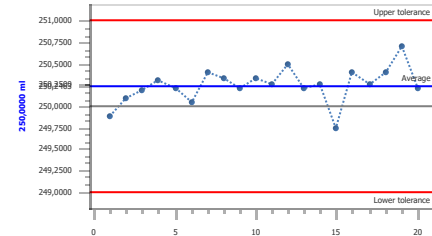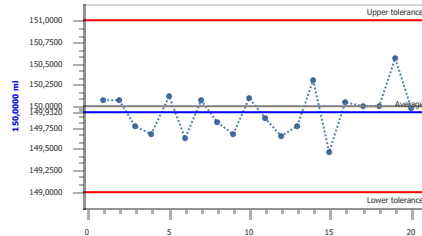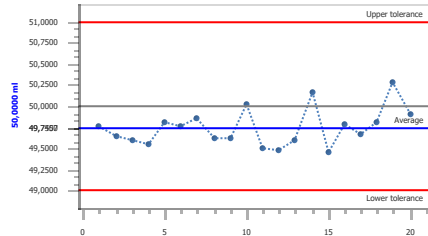

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	7
<b>Date:</b>	14.11.2023
<b>Balance:</b>	Sartorius - LA 1200 S

