

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 025 BL

Grad. cylinder, 250:2 ml, blue grad., A, conf. cert.




Batch: 22-26

Serial:

Measuring Nr. 78427

Batch size: 133

Volume:	50,0000 ml	150,0000 ml	250,0000 ml
Tolerance:	$\pm 1,0000$ ml	$\pm 1,0000$ ml	$\pm 1,0000$ ml
Average value:	49,6746 ml	149,9051 ml	250,2026 ml
Deviation:	0,1299 ml	0,0933 ml	0,0917 ml
Precision (CV):	0,2598 %	0,0622 %	0,0367 %

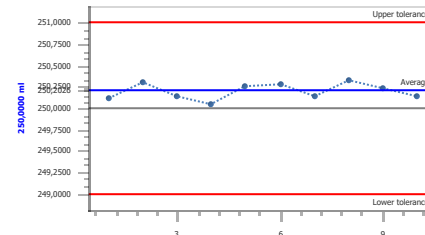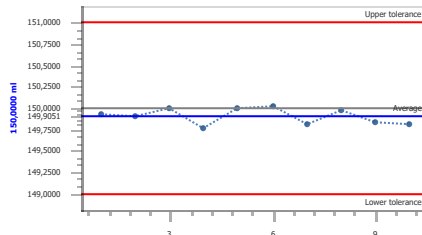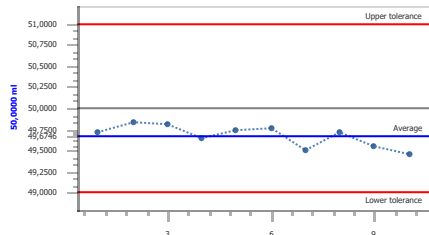

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

4

Date:

15.06.2026

Balance:

Sartorius - LA
1200 S

DE-M