

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 050 BL

Grad. cylinders, 500:5 ml, blue grad., A, conf. cert.




Batch: 30-21

Serial:

Measuring Nr.: 48071

Batch size: 280

Volume:	100,000 ml	300,000 ml	500,000 ml
Tolerance:	± 2,5000 ml	± 2,5000 ml	± 2,5000 ml
Average value:	99,7236 ml	299,9984 ml	500,0022 ml
Deviation:	0,4308 ml	0,2559 ml	0,2233 ml
Precision (CV):	0,4308 %	0,0853 %	0,0447 %

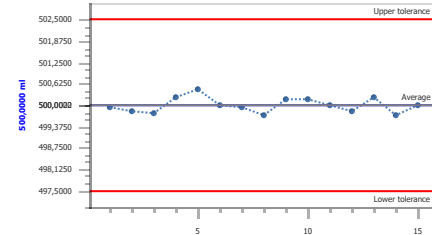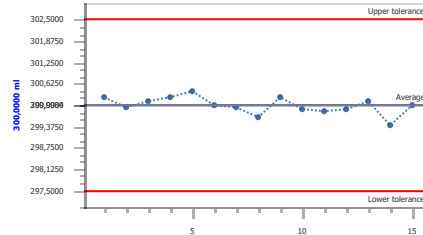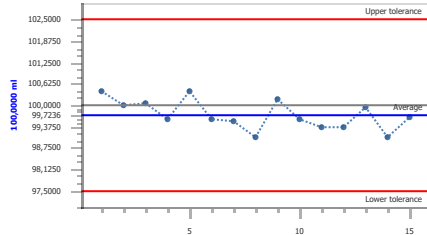

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	26.07.2021
Balance:	Sartorius - LA 1200 S

