

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 715 050 BL

**Grad. cylinder, 500:5 ml, blue grad., A, conf. cert.**




**Batch:** 44-22

**Serial:**

**Measuring Nr.** 60140

**Batch size:** 280

Volume:	100,000 ml	300,000 ml	500,000 ml
<b>Tolerance:</b>	± 2,5000 ml	± 2,5000 ml	± 2,5000 ml
<b>Average value:</b>	99,9925 ml	300,1187 ml	499,9861 ml
<b>Deviation:</b>	0,5980 ml	0,4222 ml	0,3149 ml
<b>Precision (CV):</b>	0,5980 %	0,1407 %	0,0630 %

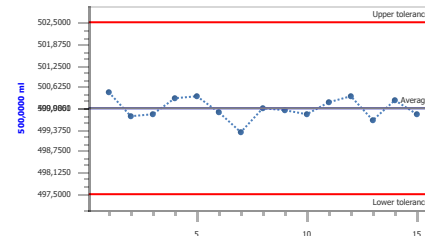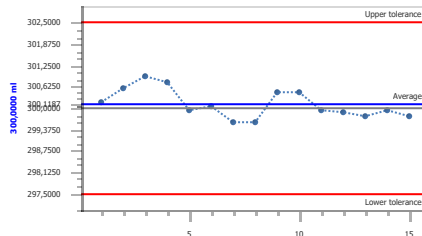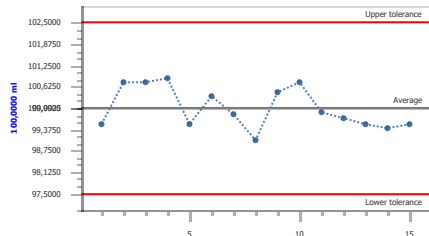

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	4
<b>Date:</b>	07.11.2022
<b>Balance:</b>	Sartorius - LA 1200 S

