

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 050

Graduated cylinder, 500:5 ml, A, conf. cert.




Batch: 11-20

Serial:

Measuring Nr. 36688

Batch size: 500

Volume:	100,000 ml	300,000 ml	500,000 ml
Tolerance:	± 2,5000 ml	± 2,5000 ml	± 2,5000 ml
Average value:	100,1718 ml	300,2542 ml	500,2956 ml
Deviation:	0,2581 ml	0,2732 ml	0,3826 ml
Precision (CV):	0,2581 %	0,0911 %	0,0765 %

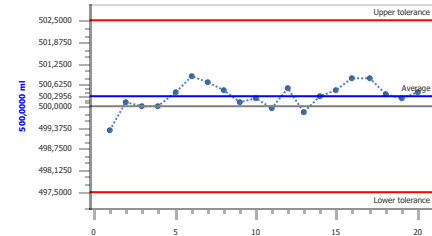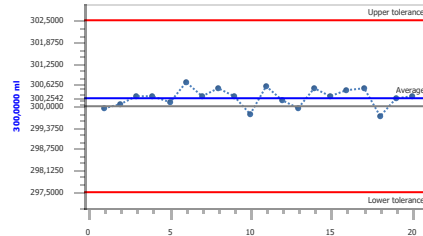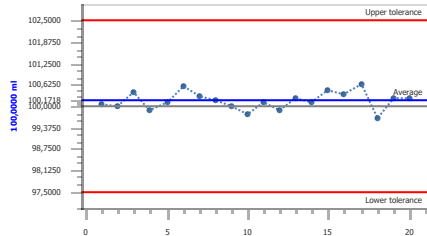

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	18.03.2020
Balance:	Sartorius - LA 1200 S

