

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 050

Graduated cylinder, 500:5 ml, A, conf. cert.




Batch: 44-20

Serial:

Measuring Nr.: 42085

Batch size: 900

Volume:	100,000 ml	300,000 ml	500,000 ml
Tolerance:	± 2,5000 ml	± 2,5000 ml	± 2,5000 ml
Average value:	100,1772 ml	300,0157 ml	499,7603 ml
Deviation:	0,4691 ml	0,3456 ml	0,2732 ml
Precision (CV):	0,4691 %	0,1152 %	0,0546 %

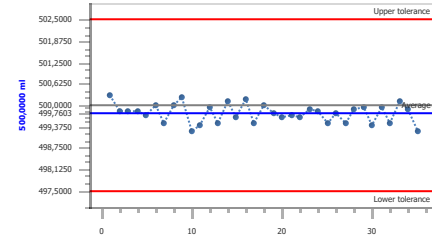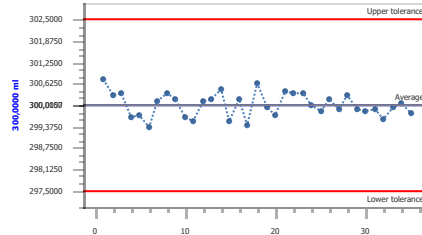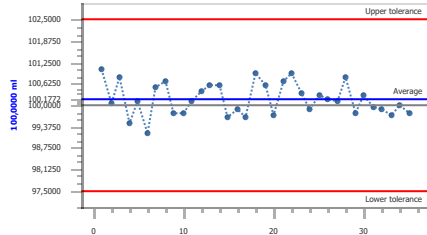

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

4

Date:

02.11.2020

Balance:

Sartorius - LA
1200 S

DE-M