

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 715 100 BL

**Grad. cylinder, 1000:10 ml, blue grad., A, conf. cert.**




**Batch:** 26-20

**Serial:**

**Measuring Nr.:** 38974

**Batch size:** 100

Volume:	200,000 ml	600,000 ml	1000,000 ml
<b>Tolerance:</b>	± 5,0000 ml	± 5,0000 ml	± 5,0000 ml
<b>Average value:</b>	199,5073 ml	599,8197 ml	999,8059 ml
<b>Deviation:</b>	0,8393 ml	1,3952 ml	0,8529 ml
<b>Precision (CV):</b>	0,4197 %	0,2325 %	0,0853 %

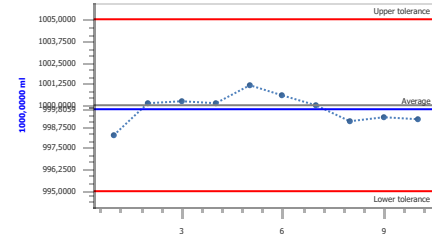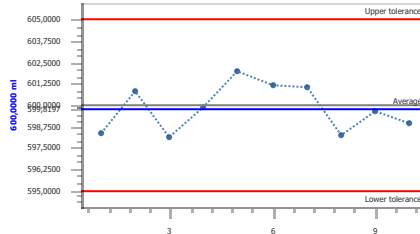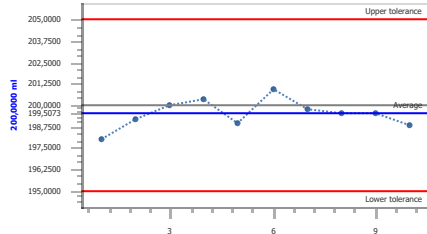

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	9
<b>Date:</b>	02.07.2020
<b>Balance:</b>	Sartorius - LC 6200 S

