

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 100 BL

Grad. cylinder, 1000:10 ml, blue grad., A, conf. cert.




Batch: 41-20

Serial:

Measuring Nr. 40940

Batch size: 150

Volume:	200,000 ml	600,000 ml	1000,000 ml
Tolerance:	± 5,0000 ml	± 5,0000 ml	± 5,0000 ml
Average value:	199,9683 ml	599,5233 ml	998,8560 ml
Deviation:	0,5023 ml	0,6589 ml	0,4920 ml
Precision (CV):	0,2512 %	0,1098 %	0,0492 %

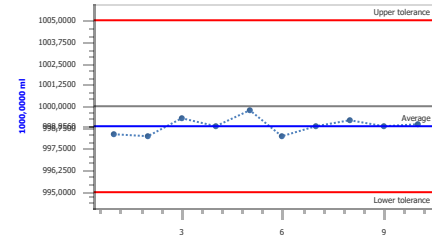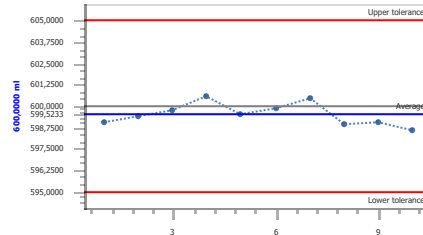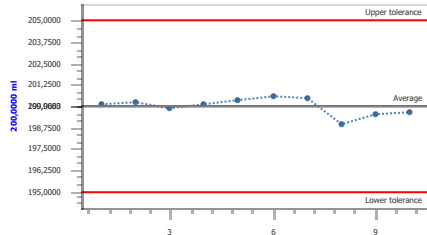

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	07.10.2020
Balance:	Sartorius - LC 6200 S

