Certificate of performance


witeg GERMANY


ISO 9001 CERTIFIED


Article:	**3 715 100**
Graduated cylinder, 1000:10 ml, A, conf. cert.	

Batch:	39-26	**Serial:**	
Measuring Nr.	80166	**Batch size:**	500

Volume:	**200,0000 ml**	**600,0000 ml**	**1000,0000 ml**
Tolerance:	± 5,0000 ml	± 5,0000 ml	± 5,0000 ml
Average value:	199,9704 ml	600,2167 ml	1000,6151 ml
Deviation:	0,4263 ml	0,5209 ml	0,4633 ml
Precision (CV):	0,2132 %	0,0868 %	0,0463 %

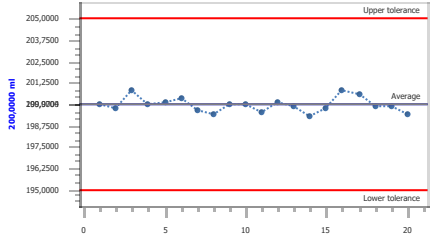

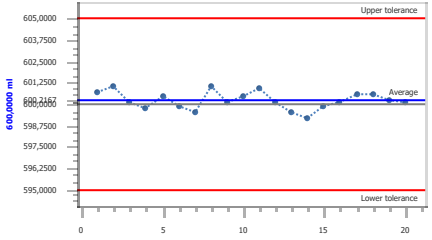

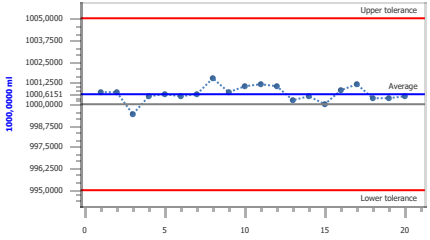

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH
Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	09.10.2026
Balance:	Sartorius - MSE14202S-0CE-D0

DE-M