

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 715 200 USP

**Graduated cylinder, 2000:20 ml, USP, A, conf. cert.**




**Batch:** 03-18

**Serial:**

**Measuring Nr.** 17184

**Batch size:** 23

Volume:	400,000 ml	1200,000 ml	2000,000 ml
<b>Tolerance:</b>	± 6,0000 ml	± 6,0000 ml	± 6,0000 ml
<b>Average value:</b>	401,1593 ml	1199,0707 ml	1997,2797 ml
<b>Deviation:</b>	1,7200 ml	1,6441 ml	0,5821 ml
<b>Precision (CV):</b>	0,4300 %	0,1370 %	0,0291 %

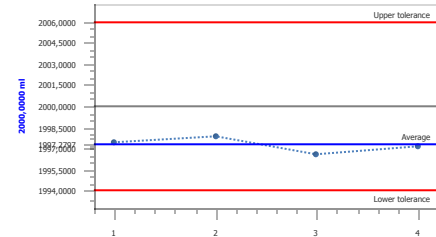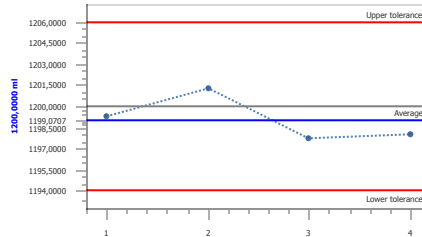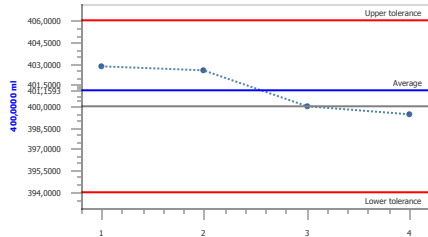

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	4
<b>Date:</b>	18.01.2018
<b>Balance:</b>	Sartorius - LC 6200 S

