

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 200 USP

Graduated cylinder, 2000:20 ml, USP, A, conf. cert.




Batch: 30-22

Serial:

Measuring Nr. 57685

Batch size: 20

Volume:	400,000 ml	1200,000 ml	2000,000 ml
Tolerance:	± 6,0000 ml	± 6,0000 ml	± 6,0000 ml
Average value:	400,3558 ml	1199,5669 ml	1999,6713 ml
Deviation:	0,2077 ml	0,4240 ml	0,9116 ml
Precision (CV):	0,0519 %	0,0353 %	0,0456 %

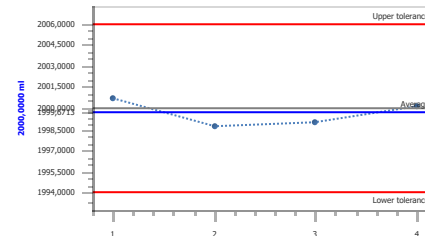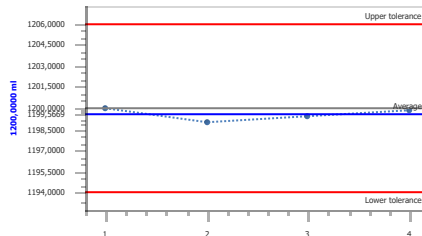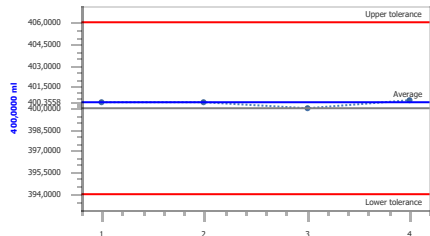

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	28.07.2022
Balance:	Sartorius - LC 6200 S

