

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 200 USP

Graduated cylinder, 2000:20 ml, USP, A, conf. cert.




Batch: 32-24

Serial:

Measuring Nr. 68611

Batch size: 50

Volume:	400,000 ml	1200,000 ml	2000,000 ml
Tolerance:	± 6,0000 ml	± 6,0000 ml	± 6,0000 ml
Average value:	400,4457 ml	1200,8872 ml	2001,3368 ml
Deviation:	0,6581 ml	0,6543 ml	0,4191 ml
Precision (CV):	0,1645 %	0,0545 %	0,0210 %

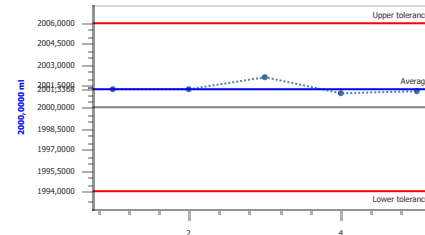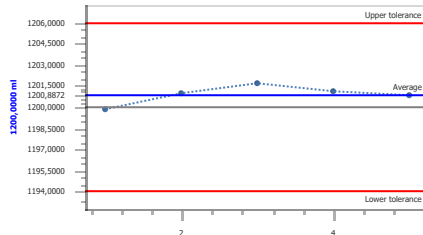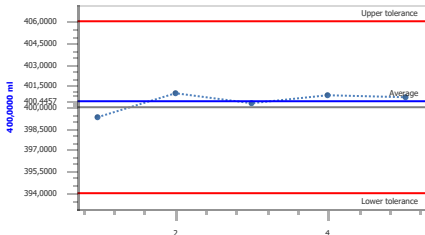

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	15.08.2024
Balance:	Sartorius - MSE14202S- OCE-D0

