

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 715 200

**Graduated cylinder, 2000:20 ml, A, conf. cert.**




**Batch:** 19-20

**Serial:**

**Measuring Nr.** 38077

**Batch size:** 146

Volume:	400,000 ml	1200,000 ml	2000,000 ml
<b>Tolerance:</b>	± 10,0000 ml	± 10,0000 ml	± 10,0000 ml
<b>Average value:</b>	397,5708 ml	1198,2644 ml	1999,2718 ml
<b>Deviation:</b>	1,1976 ml	1,0882 ml	0,8871 ml
<b>Precision (CV):</b>	0,2994 %	0,0907 %	0,0444 %

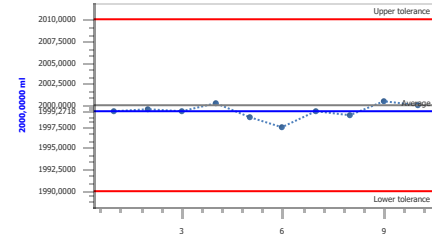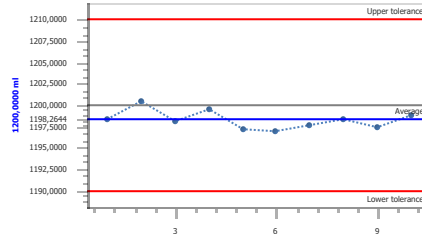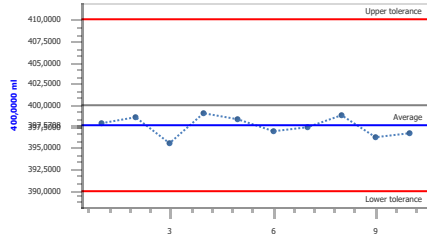

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	4
<b>Date:</b>	20.05.2020
<b>Balance:</b>	Sartorius - LC 6200 S

