

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 200

Graduated cylinder, 2000:20 ml, A, conf. cert.




Batch: 45-21

Serial:

Measuring Nr.: 50461

Batch size: 150

Volume:	400,000 ml	1200,000 ml	2000,000 ml
Tolerance:	± 10,000 ml	± 10,000 ml	± 10,000 ml
Average value:	399,0868 ml	1199,0407 ml	1998,9657 ml
Deviation:	1,7570 ml	1,6079 ml	2,1007 ml
Precision (CV):	0,4393 %	0,1340 %	0,1050 %

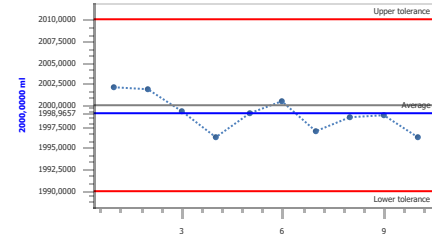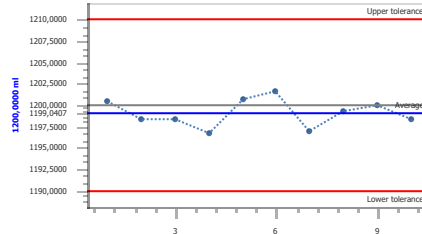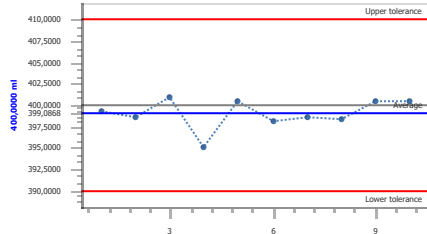

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	15.11.2021
Balance:	Sartorius - LC 6200 S

