

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 200

Graduated cylinder, 2000:20 ml, A, conf. cert.




Batch: 15-26

Serial:

Measuring Nr.: 77307

Batch size: 120

Volume:	400,000 ml	1200,000 ml	2000,000 ml
Tolerance:	± 10,0000 ml	± 10,0000 ml	± 10,0000 ml
Average value:	400,1862 ml	1199,4227 ml	1998,4296 ml
Deviation:	2,4246 ml	2,0658 ml	1,6542 ml
Precision (CV):	0,6061 %	0,1722 %	0,0827 %

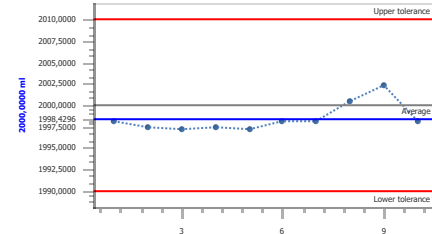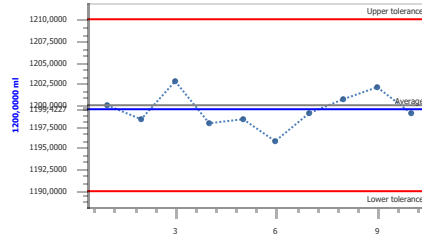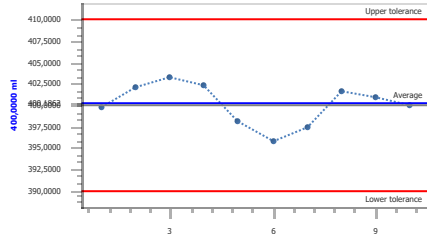

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	10.04.2026
Balance:	Sartorius - MSE14202S- OCE-D0

