

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 754 005 BL

Grad. cylinder, 50:1 ml, NS 19, blue grad., A, conf. cert.




Batch: 48-18

Serial:

Measuring Nr. 26222

Batch size: 236

Volume:	10,000 ml	30,000 ml	50,000 ml
Tolerance:	± 0,5000 ml	± 0,5000 ml	± 0,5000 ml
Average value:	10,0002 ml	30,0274 ml	50,0514 ml
Deviation:	0,0467 ml	0,0338 ml	0,0163 ml
Precision (CV):	0,4666 %	0,1128 %	0,0326 %

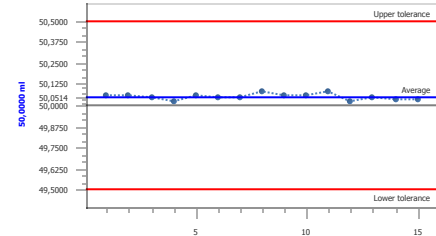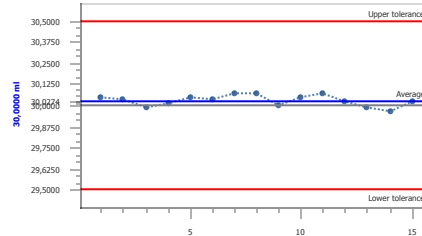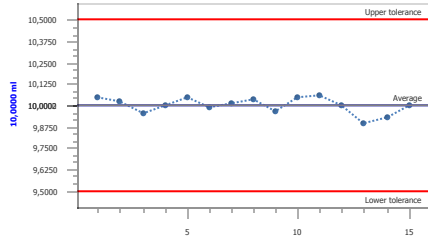

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	05.12.2018
Balance:	Sartorius - LE244S-OCE

