

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 005 BL

Vol. flasks, 50 ml, NS 12, blue grad., A, conf. cert.


Batch: 12-20

Serial:

Measuring Nr. 37319

Batch size: 4941

Volume:	50,0000 ml
Tolerance:	$\pm 0,0600$ ml
Average value:	49,9939 ml
Deviation:	0,0085 ml
Precision (CV):	0,0171 %

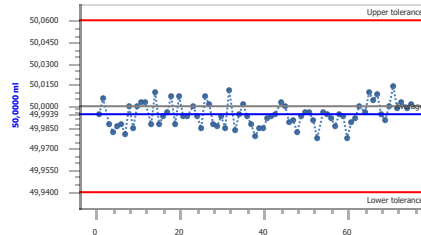

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	16.04.2020
Balance:	Sartorius - MSE224S-0CE -DU

DE-M