

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 010 BL

Vol. flasks, 100 ml, NS 12, blue grad., A, conf. cert.

Batch: 46-24


Serial:

Measuring Nr. 70504

Batch size:

2214

Volume:	100,000 ml
Tolerance:	$\pm 0,1000$ ml
Average value:	100,0147 ml
Deviation:	0,0204 ml
Precision (CV):	0,0204 %

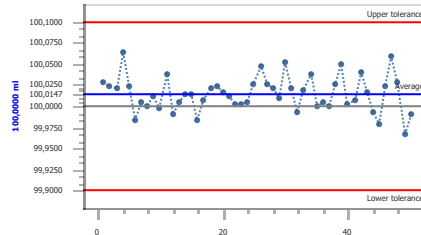

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

77

Date:

22.11.2024

Balance:

Sartorius -
MSE224S-0CE
-DU

DE-M