

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 020 BL USP

Vol. flask, 200 ml, NS 14, blue grad., USP, A, conf. cert.


Batch: 35-23

Serial:

Measuring Nr. 64314

Batch size: 150

Volume:	200,000 ml
Tolerance:	$\pm 0,1000$ ml
Average value:	200,0315 ml
Deviation:	0,0271 ml
Precision (CV):	0,0135 %

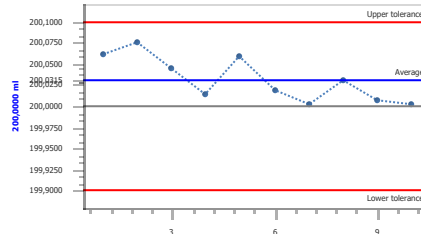

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	04.09.2023
Balance:	Sartorius - LA 1200 S

DE-M