

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 662 020 BL USP

**Vol. flask, 200 ml, NS 14, blue grad., USP, A, conf. cert.**


**Batch:** 32-25

**Serial:**

**Measuring Nr.** 74173

**Batch size:** 150

<b>Volume:</b>	200,000 ml
<b>Tolerance:</b>	$\pm 0,1000$ ml
<b>Average value:</b>	200,0254 ml
<b>Deviation:</b>	0,0114 ml
<b>Precision (CV):</b>	0,0057 %

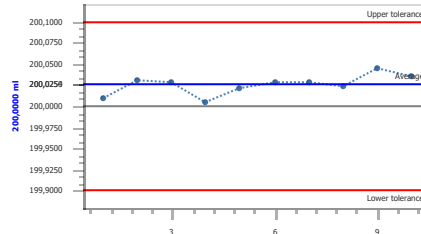

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	7
<b>Date:</b>	14.08.2025
<b>Balance:</b>	Sartorius - LA 1200 S

DE-M