

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 025 BL

Vol. flask, 250 ml, NS 14, blue grad., A, conf. cert.

Batch: 23-26

Serial:

Measuring Nr. 78437

Batch size: 487


Volume: 250,0000 ml

Tolerance: $\pm 0,1500$ ml

Average value: 249,9883 ml

Deviation: 0,0281 ml

Precision (CV): 0,0112 %

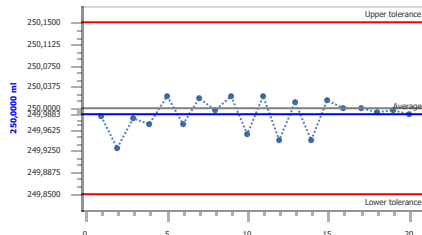

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

4

Date:

15.06.2026

Balance:

Sartorius - LA
1200 S

DE-M