

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 100 USP

Volumetric flask, 1000 ml, NS 24, USP, A, conf. cert.

Batch: 50-25


Serial:

Measuring Nr. 76185

Batch size:

147

| | |
|------------------------|--------------|
| Volume: | 1000,0000 ml |
| Tolerance: | ± 0,3000 ml |
| Average value: | 1000,0850 ml |
| Deviation: | 0,0417 ml |
| Precision (CV): | 0,0042 % |

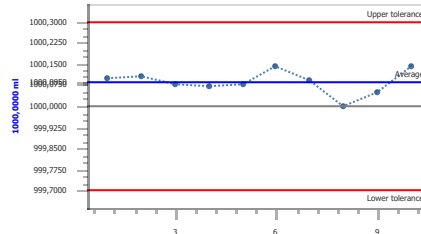

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

4

Date:

16.01.2026

Balance:

Sartorius -
MSE14202S-
OCE-D0

DE-M