

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 101 BL

Vol. flasks, 1000 ml, NS 29, blue grad., A, conf. cert.


Batch: 30-25

Serial:

Measuring Nr. 75412

Batch size: 90

Volume:	1000,000 ml
Tolerance:	$\pm 0,6000$ ml
Average value:	1000,4109 ml
Deviation:	0,0599 ml
Precision (CV):	0,0060 %

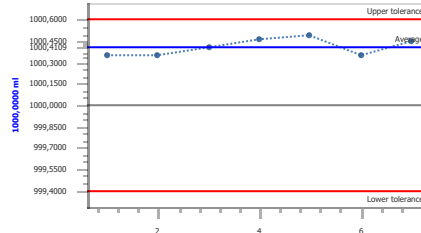

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	24.11.2025
Balance:	Sartorius - MSE14202S- OCE-D0

DE-M