

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 200 BL

Vol. flask, 2000 ml, NS 29, blue grad., A, conf. cert.

Batch: 35-25


Serial:

Measuring Nr. 74875

Batch size:

189

| | |
|------------------------|-----------------|
| Volume: | 2000,0000 ml |
| Tolerance: | $\pm 0,6000$ ml |
| Average value: | 2000,3039 ml |
| Deviation: | 0,0686 ml |
| Precision (CV): | 0,0034 % |

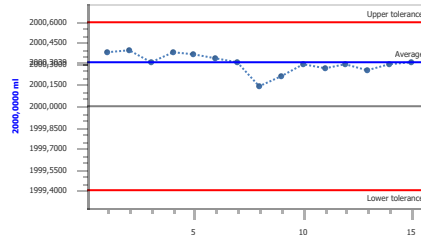

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

4

Date:

07.10.2025

Balance:

Sartorius -
MSE14202S-
OCE-D0

DE-M