

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 300 BL

Vol. flask, 3000 ml, NS 29, blue grad., A, conf. cert.

Batch: 49-17


Serial:

Measuring Nr. 16782

Batch size:

6

Volume:	3000,0000 ml
Tolerance:	$\pm 0,8000$ ml
Average value:	3000,1549 ml
Deviation:	0,1383 ml
Precision (CV):	0,0046 %

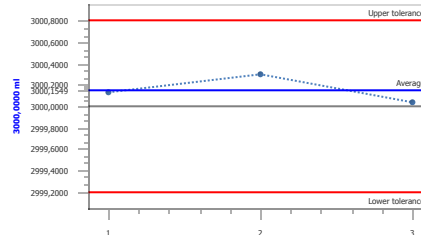

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

4

Date:

21.12.2017

Balance:

Sartorius - LC
6200 S

DE-M